



ENSURING THE
EXPERTISE TO GROW
SOUTH AFRICA

**Sub Discipline-specific Training Guideline for Candidate
Medical Equipment Maintainers**

R-05-MEM-SC

REVISION 0: 09 February 2022



Document No.: R-05-MEM-SC	Revision No.: 0	Effective Date: 09/02/2022	
Subject: Sub Discipline-specific Training Guideline for Candidate Medical Equipment Maintainers			
Compiler: MB Mtshali	Approving Officer: EL Nxumalo	Next Review Date: 09/02/2026	Page 2 of 34

TABLE CONTENTS

BACKGROUND	3
1. PURPOSE OF THIS DOCUMENT	3
2. AUDIENCE	4
3. PERSONS NOT REGISTERED AS A CANDIDATE OR NOT TRAINING UNDER A C&U 7	
4. TRAINING OBJECTIVES.....	8
5. MEDICAL EQUIPMENT MAINTAINERS.....	8
6. TRAINING IMPLICATIONS OF THE NATURE AND ORGANISATION OF THE INDUSTRY	
.....	11
6.1 Specific Equipment Types Applicable to Medical Devices	11
6.2 Ability to Provide Complete Training.....	12
6.3 The problem solving experience may be obtained in any of the following work categories:	
.....	12
6.3.1 Design or Development.....	12
6.3.2 Operations	13
6.3.3 Research and Development.....	13
7. DEVELOPING COMPETENCY: ELABORATING ON SECTIONS IN THE GUIDE TO THE	
COMPETENCY STANDARD (R-08-SC)	14
7.1 Contextual Knowledge	15
7.2 Functions Performed.....	16
7.3 Industry-related statutory and other requirements	16
7.4 Recommended Formal Learning Activities	17
8. PROGRAMME STRUCTURE AND SEQUENCING	17
8.1 Best Practice.....	17
8.2 Orientation requirements.....	19
8.3 Realities	19
8.4 Considerations for generalists, specialists, researchers and academics	19
8.5 Moving into or Changing Candidacy Programmes.....	19
8.6 Compulsory Sub Discipline-specific Requirements to be met during the Candidacy.....	20
REVISION HISTORY	22
Training Elements	27

CONTROLLED DISCLOSURE

When downloaded for the ECSA Document Management System, this document is uncontrolled and the responsibility rests with the user to ensure that it is in line with the authorised version on the database. If the 'original' stamp in red does not appear on each page, this document is uncontrolled.

Document No.: R-05-MEM-SC	Revision No.: 0	Effective Date: 09/02/2022	
Subject: Sub Discipline-specific Training Guideline for Candidate Medical Equipment Maintainers			
Compiler: MB Mtshali	Approving Officer: EL Nxumalo	Next Review Date: 09/02/2026	Page 3 of 34

BACKGROUND

The documents that define the Engineering Council of South Africa (ECSCA) system for registration in specified categories are shown in **Figure 1** which also locates the current document.

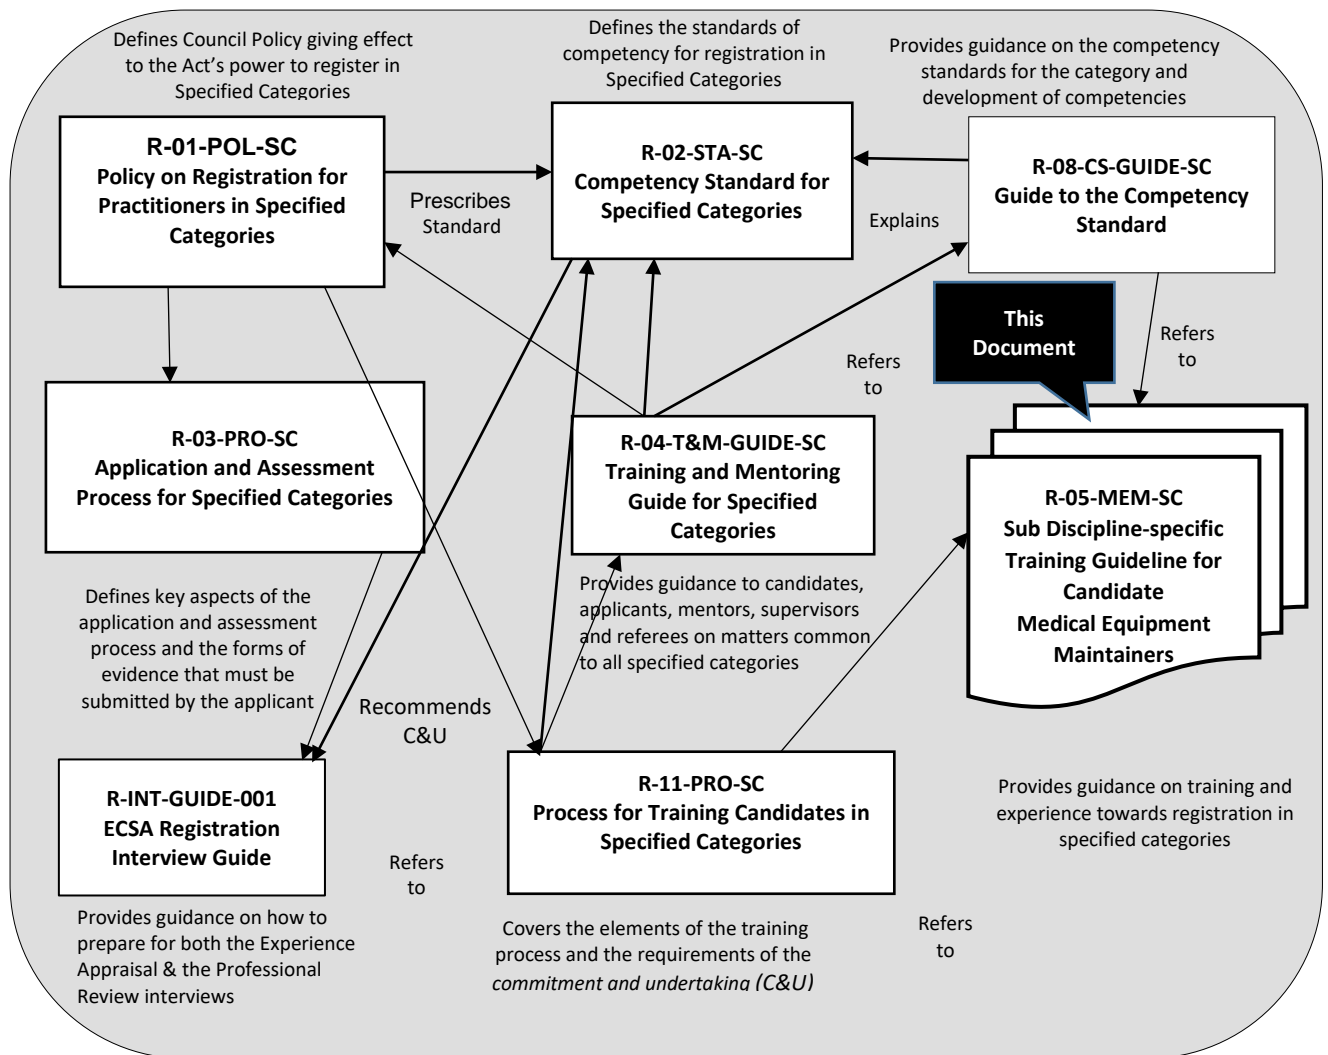



Figure 1: Documents defining the ECSCA Registration system

1. PURPOSE OF THIS DOCUMENT

All persons applying for registration in the Specified Category of Medical Equipment Maintainer are expected to demonstrate the competencies specified in document **R-02-STA-SC** at the prescribed level, irrespective of the type of medical equipment applicable, through

CONTROLLED DISCLOSURE

When downloaded for the ECSCA Document Management System, this document is uncontrolled and the responsibility rests with the user to ensure that it is in line with the authorised version on the database. If the 'original' stamp in red does not appear on each page, this document is uncontrolled.

Document No.: R-05-MEM-SC	Revision No.: 0	Effective Date: 09/02/2022	
Subject: Sub Discipline-specific Training Guideline for Candidate Medical Equipment Maintainers			
Compiler: MB Mtshali	Approving Officer: EL Nxumalo	Next Review Date: 09/02/2026	Page 4 of 34

work performed by the applicant at the prescribed level of responsibility. In addition, the Sub-discipline Specific Requirements set out in 8.6 below must be met.

This document supplements the generic Training and Mentoring Guide **R-04-T&M-GUIDE-SC**, Guide to the Competency Standards for Registered Specified Category Practitioners **R-08-CS-GUIDE-SC** .and Process for Training Engineering Candidates towards Specified Category Registration **R-11-PRO-SC**.

In document **R-04-T&M-GUIDE-SC** attention is drawn to the following sections:

- Duration of training and period working at level required for registration
- Principles of planning training and experience
- Progression of Training programme
- Documenting Training and Experience
- Demonstrating responsibility

The second document **R-08-CS-GUIDE-SC** provides both a high-level and outcome-by-outcome understanding of the competency standards as an essential basis for this sub-discipline-specific training requirements document.

The third document **R-11-PRO-SC** elaborates on the elements of the training process and the requirements of the Commitment and Undertaking.


These Requirements, as well as **R-04-T&M-GUIDE-SC**, **R-08-CS-GUIDE-SC** and **R-11-PRO-SC**, are subordinate to the Policy on Registration, document **R-01-POL-SC**, the Competency Standard (**R-02-STA-SC**) and the application process definition (**R-03-PRO-SC**).

2. AUDIENCE

In the first instance, these Requirements are directed to candidates and their supervisors and mentors in the sub-discipline of Medical Equipment Maintainers. The Requirements are intended to support a programme of training and experience incorporating good practice elements.

CONTROLLED DISCLOSURE

When downloaded for the ECSA Document Management System, this document is uncontrolled and the responsibility rests with the user to ensure that it is in line with the authorised version on the database. If the 'original' stamp in red does not appear on each page, this document is uncontrolled.

Document No.: R-05-MEM-SC	Revision No.: 0	Effective Date: 09/02/2022	
Subject: Sub Discipline-specific Training Guideline for Candidate Medical Equipment Maintainers			
Compiler: MB Mtshali	Approving Officer: EL Nxumalo	Next Review Date: 09/02/2026	Page 5 of 34

In the second place, the Requirements are directed to the members of the engineering team comprising the following:

Table 1: This table contains the different categories in the engineering team of registered practitioners accepting full responsibility for their area of work and adhering to ECSA's Code of Conduct. (EPA = Engineering Professions Act (No. 46 of 2000))

Category	Authority	Underpinning Knowledge	Area of Responsibility
Professional Engineer (EPA Section 18(1)(a)(i))	Educated, trained and experienced to carry out complex-defined engineering work.	Graduate Attributes acquired in education at NQF 8 level (560 credits)	Complex interaction between professions and disciplines. Justify work outside codes, standards and procedures.
Professional Certificated Engineer (EPA Section 18(1)(a)(iii))	Educated, trained and experienced to carry out broadly-defined engineering work	Graduate Attributes acquired in education at NQF 7 level (420 credits) and Government Certificate of Competency	Interaction with other professions and disciplines. Authorisation required to work outside codes, standards and procedures after conducting research and investigation. Legal responsibility (OH&S Act)
Professional Engineering Technologist (EPA Section 18(1)(a)(ii))	Educated, trained and experienced to carry out broadly-defined engineering work	Graduate Attributes acquired in education at NQF 7 level (420 credits)	Interaction with other professions and disciplines. Authorisation required to work outside codes, standards and procedures after conducting research and investigation.
Professional Engineering Technician (EPA Section 18(1)(a)(iv))	Educated, trained and experienced to carry out well-defined engineering work	Graduate Attributes acquired in education at NQF 6 level (280 to 360 credits)	Mostly working within a single discipline. Strict adherence to codes, standards and procedures. Repetitive work.
Specified Category Practitioner (EPA Section 18(1)(c))	Educated, trained and experienced to carry out specifically-defined engineering work	Graduate Attributes acquired in education at NQF 5 level (140 credits)	Working within a single discipline in a specific field. May be legally responsible for work.

These Requirements apply to persons who have:


1. Completed the education requirements by the Benchmark or Engineering Management Pathways in Table 2.

Table 2: Minimum duration of education, training and experience for various pathways towards registration:

Pathway	Qualification	Post Qualification Total Training and Experience in the Specific Discipline	Post Qualification Experience (part of total) with Responsibility as Indicated
Experience Route (Alternative Route)	No Tertiary Qualification	NQF 1 level: 20 years NQF 2 level: 15 years NQF 3 level: 10 years NQF 4 level: 5 years	2 years test and inspection or commissioning

CONTROLLED DISCLOSURE

When downloaded for the ECSA Document Management System, this document is uncontrolled and the responsibility rests with the user to ensure that it is in line with the authorised version on the database. If the 'original' stamp in red does not appear on each page, this document is uncontrolled.


Document No.: R-05-MEM-SC	Revision No.: 0	Effective Date: 09/02/2022	
Subject: Sub Discipline-specific Training Guideline for Candidate Medical Equipment Maintainers			
Compiler: MB Mtshali	Approving Officer: EL Nxumalo	Next Review Date: 09/02/2026	Page 6 of 34

Pathway	Qualification	Post Qualification Total Training and Experience in the Specific Discipline	Post Qualification Experience (part of total) with Responsibility as Indicated
Benchmark Route	Higher Certificate in Engineering or Equivalent (NQF 5) or Completed Apprenticeship in an Acceptable Trade (up to 4 years)	NQF 5 level: 3 years	2 years inspection, testing, commissioning, handover, certification, etc.
Engineering Management Type Route	BSc (Eng), BEng, BTech, N Dip, Advanced Certificate or Equivalent but not eligible for ECSA registration in any of the Professional Categories	NQF 6 level: 3 years NQF 7 level: 3 years NQF 8 level: 3 years	2 years planning, organising, leading, implementing and controlling engineering activities, including design control and approval, budget compilation and control, quality, environmental, safety and society management, legal matters, skills development, report and instruction writing, meeting management, ethics, etc.
Notes:	<ul style="list-style-type: none"> a. Training and experience must incorporate legal requirements stipulated in laws, regulations and standards applicable (As detailed in the Sub Discipline-specific Training Requirements (SDSTR's) R-05-nnn-SC). b. Training and experience must incorporate practical requirements detailed by equipment manufacturers, codes of practice, etc. applicable to the specific field (As detailed in the SDSTR's R-05-nnn-SC). c. Academic programmes referred to above must be accredited, recognised or evaluated as equivalent, with individual assessment where required. d. Equivalent refers to Equivalent Qualifications to the qualification(s) listed, e.g. past and future qualifications developed by education providers (QCTO, TVET) and accredited or recognised by ECSA.. 		

2. Met the Educational Requirements via the Alternative Route Pathway in Table 2; the evaluation/assessment as detailed in document **E-17-PRO-SC**. If the applicant does not have at least the benchmark academic qualification (HCert, or equivalent or a Completed Apprenticeship), their application will be considered by the **alternate route**. The difference must be made up by extended periods of engineering experience. The exact periods will depend upon the level of qualifications held by the applicant. The work which the candidates are doing or have done, as well as the submission of correctly completed Training and Experience Reports and the Engineering Report

CONTROLLED DISCLOSURE

When downloaded for the ECSA Document Management System, this document is uncontrolled and the responsibility rests with the user to ensure that it is in line with the authorised version on the database. If the 'original' stamp in red does not appear on each page, this document is uncontrolled.

Document No.: R-05-MEM-SC	Revision No.: 0	Effective Date: 09/02/2022	
Subject: Sub Discipline-specific Training Guideline for Candidate Medical Equipment Maintainers			
Compiler: MB Mtshali	Approving Officer: EL Nxumalo	Next Review Date: 09/02/2026	Page 7 of 34

(Forms TER/TEO-SC and ER-SC respectively) and the Initial Professional Development Report (Form IPD-SC), must also incorporate developmental evidence of meeting the educational requirements.

3. Registered as Candidate Specified Category;
4. Embarked on a process of acceptable training under a registered **Commitment and Undertaking (C&U)** with a Mentor guiding the professional development process at each stage.

3. PERSONS NOT REGISTERED AS A CANDIDATE OR NOT TRAINING UNDER A C&U

All applicants for registration must present the same evidence of competence and be assessed against the same standards and requirements, irrespective of the development path followed. Application for registration as a Specified Category Practitioner is permitted without being registered as a Candidate Specified Category or without training under a C&U. Mentorship and adequate supervision are however key factors in effective development to the level required for registration. A C&U indicates that the company is committed to mentorship and supervision.


If the trainee's employer has no C&U, the trainee should establish the level of mentorship and supervision the employer is able to provide. In the absence of an internal mentor, the services of an external mentor should be secured. The recognised Voluntary Association (VA) for the sub discipline should be consulted for assistance in locating an external mentor. A mentor should be in place at all stages of the development process.

These Requirements are written for the recent graduate who is training and gaining experience toward registration. Mature applicants for registration may apply the guide retrospectively to identify possible gaps in their development.

Any applicants who have not enjoyed mentorship are advised to request an experienced mentor (internal or external) to act as an application adviser while they prepare their application for registration.

CONTROLLED DISCLOSURE

When downloaded for the ECSA Document Management System, this document is uncontrolled and the responsibility rests with the user to ensure that it is in line with the authorised version on the database. If the 'original' stamp in red does not appear on each page, this document is uncontrolled.

Document No.: R-05-MEM-SC	Revision No.: 0	Effective Date: 09/02/2022	
Subject: Sub Discipline-specific Training Guideline for Candidate Medical Equipment Maintainers			
Compiler: MB Mtshali	Approving Officer: EL Nxumalo	Next Review Date: 09/02/2026	Page 8 of 34

These Requirements may be applied in the case of a person moving into a candidacy programme at a later stage that is at a level below that required for registration (see **Section 8.5**).

4. TRAINING OBJECTIVES

To achieve ECSA registration the trainee's employer should design the training program to achieve the following:

- 4.1 Expose the applicant to experience and training enabling him or her to apply engineering theory acquired during educational development to practical workplace situations for the prescribed period required.
- 4.2 Incorporate an increasing level of responsibility to enable the applicant to submit evidence in the training and experience reports of achieving the duration and level detailed in **Section 8.1**.
- 4.3 Develop the engineering competency of the applicant to cover the eleven outcomes in the five major groups referred to in **Section 7.2 and Appendix B**, and the discipline specific requirements referred to **Section 8.6**.


5. MEDICAL EQUIPMENT MAINTAINERS

In today's healthcare market, technology is paramount. The need for a workforce knowledgeable in the theory of operation, underlying physiological principles, and safe application of biomedical equipment is a central concern of many hospitals and companies. Registration with ECSA demonstrates that successful applicants have the knowledge to ensure a safe, reliable healthcare environment. It also demonstrates to employers a significant commitment to career and competence.

Registered *Medical Equipment Maintainers (MEM's)* conduct problem solving in the design, installation, commissioning, maintenance and inspection of a range of medical equipment, applying scientific and engineering skills to do so. In this process communication is of paramount importance, including adherence to legislation and acceptance of a high degree of ethical behaviour. In executing his or her duties the MEM must guarantee that patient safety is never compromised by ensuring total compliance with all regulations, rules and guidelines

CONTROLLED DISCLOSURE

When downloaded for the ECSA Document Management System, this document is uncontrolled and the responsibility rests with the user to ensure that it is in line with the authorised version on the database. If the 'original' stamp in red does not appear on each page, this document is uncontrolled.

Document No.: R-05-MEM-SC	Revision No.: 0	Effective Date: 09/02/2022	
Subject: Sub Discipline-specific Training Guideline for Candidate Medical Equipment Maintainers			
Compiler: MB Mtshali	Approving Officer: EL Nxumalo	Next Review Date: 09/02/2026	Page 9 of 34

pertaining to medical equipment. Hospital staff must have confidence in the equipment, and management must feel that they are receiving a competent service and value for money. If medical service providers are compelled to employ registered MEM practitioners, such appointed persons must be held responsible/accountable in the event of unacceptable service.

The responsibility for ensuring the safety of patients (the general public) through appropriate protective legislation lies with the Department of Health. It is thus imperative that regulations formulated in response, apply across the board, i.e. both public and private institutions.

The external and internal stakeholders in the MEM environment are the following:


- Department of National Health (internal);
- Clinical Engineering Association of South Africa;
- Vendor companies delivering service and supplying high technology equipment to all medical equipment users: e.g. hospitals, medical practitioners, auxiliary medical service providers, etc.;
- Educational institutions; e.g. Tshwane University of Technology Engineering Faculty; UCT; etc.;
- All Healthcare Providers – Public and Private hospitals, clinics, treatment centres, etc.;
- Facilities Management personnel (SAFHE).

The Medical Devices Regulating Authority (MDRA) shall, subject to the provisions of the National Health Act of 2003 and the Regulations, provide for the evaluation, registration, control, regulation, monitoring and investigation of medical devices and related matters, which are in the public interest, in an efficient, effective and ethical manner that is fair, transparent and objective.

All medical devices manufactured in or imported into South Africa, taking into account of the intended purpose, must comply with the Essential Principles for Safety and Performance as set out in the appropriate Global Harmonising Task Force (GHTF) document. Medical devices are classified into low risk (Class I), low to medium risk (Class IIa), medium to high risk (Class IIb), high risk (Class III) and active implantable medical device – high risk (Class AMID). In

CONTROLLED DISCLOSURE

When downloaded for the ECSA Document Management System, this document is uncontrolled and the responsibility rests with the user to ensure that it is in line with the authorised version on the database. If the 'original' stamp in red does not appear on each page, this document is uncontrolled.

Document No.: R-05-MEM-SC	Revision No.: 0	Effective Date: 09/02/2022	
Subject: Sub Discipline-specific Training Guideline for Candidate Medical Equipment Maintainers			
Compiler: MB Mtshali	Approving Officer: EL Nxumalo	Next Review Date: 09/02/2026	Page 10 of 34

Vitro Diagnostic Devices (IVD) are classified separately into low personal risk (Class 1 IVD), low public health risk medium personal risk (Class 2 IVD), moderate public health risk high personal risk (Class 3 IVD) and high public health risk (Class 4 IVD).

For any medical device in Class IIa and higher and Class 2 and higher:

- The quality system that applies to the manufacture must be certified by a recognised certification body according to SANS/ISO 13485; and
- A risk management system according to SANS/ISO 14971:2000 must be applied

This procedure must also be applicable in respect of any medical device in Class I with a measuring function or requiring sterility.


The MEM shall keep a record of every medical device, of class IIa and higher, provided to a user/owner. The record shall include at least the following data:

- Name and contact details of the manufacturer;
- Name and contact details of the supplier;
- Make, model and serial number of the medical device;
- Accessories, upgrades, modifications and consumables for the medical device;
- Purchaser's name, physical address, telephone number, e-mail address and contact person;
- Date of provision and date of commissioning of the medical device.

The MEM must keep a record of every defect and/or adverse event in relation to a medical device registered to him/her that the MEM becomes aware of as well as the steps taken to address such defect or adverse event. A documented procedure to handle complaints must be in place. Storage, handling, transport, delivery, installation and commissioning of medical devices must be according to the manufacturer's instructions. Personnel, facilities, appropriate test equipment and tools must be locally available for calibration, maintenance, service and repair of all medical devices registered in the name of the MEM. The MEM must ensure that personnel working on medical devices have received appropriate training and are competently qualified, and that the users of the equipment receive training to correctly operate the medical devices.

CONTROLLED DISCLOSURE

When downloaded for the ECSA Document Management System, this document is uncontrolled and the responsibility rests with the user to ensure that it is in line with the authorised version on the database. If the 'original' stamp in red does not appear on each page, this document is uncontrolled.

Document No.: R-05-MEM-SC	Revision No.: 0	Effective Date: 09/02/2022	
Subject: Sub Discipline-specific Training Guideline for Candidate Medical Equipment Maintainers			
Compiler: MB Mtshali	Approving Officer: EL Nxumalo	Next Review Date: 09/02/2026	Page 11 of 34

Any person who calibrates, maintains, services, repairs or in any way works on a medical device in Class IIa and higher must be competent to do so and must have received adequate training for the particular device or be supervised by a person trained and competent in such work. Such person must be registered with an appropriate body such as the Engineering Council of South Africa. If a serious adverse event occurs during the use of a registered medical device the owner shall report the event to both the MDRA and the registered person of the device. The device shall be immediately sealed and isolated, with relevant accessories and consumables and settings intact.

6. TRAINING IMPLICATIONS OF THE NATURE AND ORGANISATION OF THE INDUSTRY

Medical Equipment Maintainers may be employed in both the private and public sector.

Typically in the private sector they would be involved in contracting, or in supplier or manufacturing organisations. Engineering contractors are responsible for project implementation and activities include planning, construction, labour and resource management. Those working in supply or manufacturing companies could be involved in research and development, and would be involved in production, supply and quality control.

The public sector is responsible for service delivery and is usually the client, though in some departments construction is also performed. Medical Equipment Maintainers are required at all levels of the public sector, including at national, provincial and local government level, state owned enterprises (SOEs), and public utilities. Medical Equipment Maintainers in the public sector largely handles overseeing implementation, operations and maintenance of infrastructure.


An extension of the public sector would include tertiary academic institutions and research organisations.

6.1 Specific Equipment Types Applicable to Medical Devices

Depending on the nature of business of each employer, Candidate *Medical Equipment Maintainers* will select one or more of the equipment types for the purpose of registration as a

CONTROLLED DISCLOSURE

When downloaded for the ECSA Document Management System, this document is uncontrolled and the responsibility rests with the user to ensure that it is in line with the authorised version on the database. If the 'original' stamp in red does not appear on each page, this document is uncontrolled.

Document No.: R-05-MEM-SC	Revision No.: 0	Effective Date: 09/02/2022	
Subject: Sub Discipline-specific Training Guideline for Candidate Medical Equipment Maintainers			
Compiler: MB Mtshali	Approving Officer: EL Nxumalo	Next Review Date: 09/02/2026	Page 12 of 34

Medical Equipment Maintainers. The present equipment types are listed and described in **Appendix A** (page 14), with the applicable SANS or other standard given, if available.

6.2 Ability to Provide Complete Training

Depending on where the candidate is employed, there may be situations where the opportunities in-house are not sufficiently diverse to develop all the competencies required in all the groups noted in document **R-02-STA-SC** and in **Appendix B**. For example the opportunity for developing problem solving competence (including design or developing solutions) and for managing engineering activities (including implementing or constructing solutions) may not both be available to the candidate. In such cases employers are encouraged to put a secondment system in place.

It has been fairly common practice that where an organisation is not able to provide training in certain areas that secondments are arranged with other organisations, so that the candidate is able to develop all the competencies required for registration. These secondments are usually of a reciprocal nature so both employers and their respective employees get the mutual benefit from the other party. Secondments between consultants and contractors, and between the public and private sector should be possible.

Problem solving is the core of engineering. It is a logical thinking process that requires *Medical Equipment Maintainers* to apply their minds diligently in bringing solutions to technically specifically-defined problems. This process involves the analysis of medical device systems or assembly of components, and integration of various elements in engineering as applied to medical equipment through the application of basic and engineering sciences.

6.3 The problem solving experience may be obtained in any of the following work categories:


6.3.1 Design or Development

Examples of acceptable design or development include, but are not limited to:

- Modifications after obtaining approval to specifically-defined control systems on medical equipment.

CONTROLLED DISCLOSURE

When downloaded for the ECSA Document Management System, this document is uncontrolled and the responsibility rests with the user to ensure that it is in line with the authorised version on the database. If the 'original' stamp in red does not appear on each page, this document is uncontrolled.

Document No.: R-05-MEM-SC	Revision No.: 0	Effective Date: 09/02/2022	
Subject: Sub Discipline-specific Training Guideline for Candidate Medical Equipment Maintainers			
Compiler: MB Mtshali	Approving Officer: EL Nxumalo	Next Review Date: 09/02/2026	Page 13 of 34

- Modifications after obtaining approval to specifically-defined minor parts of mechanical and/or electronic components on medical devices.
- Modifications after obtaining approval to test and inspection procedures on medical equipment.

6.3.2 Operations

This would mostly deal with investigating failure or underperformance of medical equipment and the synthesis of implemented and proven solutions to avoid recurrence of the problem. In addition this category of work will also involve the practical improvement recommended for optimising the operational efficiencies. The *Medical Equipment Maintainer* must, in performing the abovementioned work, apply engineering judgment to all work he or she does in the management of operations. This include, but would not be limited to, the ability to assess design work against the following criteria:


- Conformance to design specifications, health and safety regulations.
- Ease of fabrication and assembly.
- Constructability.
- Maintainability.
- Conformance to environmental requirements.
- Ergonomic considerations.
- Life cycle costs.
- Alternative solutions

6.3.3 Research and Development

This type of work may be performed in research and product development centres of business organizations or at the academic institutions. Candidate Medical Equipment Maintainers must participate in research and development work that is predominantly of mechanical and electrical engineering nature, and this work must include application of the various aspects of engineering, including product or system testing under controlled experimental conditions.

CONTROLLED DISCLOSURE

When downloaded for the ECSA Document Management System, this document is uncontrolled and the responsibility rests with the user to ensure that it is in line with the authorised version on the database. If the 'original' stamp in red does not appear on each page, this document is uncontrolled.

Document No.: R-05-MEM-SC	Revision No.: 0	Effective Date: 09/02/2022	
Subject: Sub Discipline-specific Training Guideline for Candidate Medical Equipment Maintainers			
Compiler: MB Mtshali	Approving Officer: EL Nxumalo	Next Review Date: 09/02/2026	Page 14 of 34

7. DEVELOPING COMPETENCY: ELABORATING ON SECTIONS IN THE GUIDE TO THE COMPETENCY STANDARD (R-08-SC)

Applicants are required to demonstrate the insight and ability to use and interface various aspects through verifiable performance in providing engineered solutions to practical specifically-defined problems experienced in their operating work environment. In addition applicants must develop the skills required to demonstrate the use of applicable engineering knowledge in optimizing the efficiency of operations.

Candidate Medical Equipment Maintainers must be able to demonstrate that they have been actively involved in an electrical and/or mechanical work shop environment participating in the execution of practical work such that they have learnt sufficient details on basic electrical/mechanical procedures to be able to exercise judgment in the workplace thereafter.

What is a sufficiently specifically-defined engineering (Appendix B) problem?

We can summarise the definition of *specifically-defined* in *specifically-defined engineering problems* as follows:


"Composed of ***inter-related conditions***; requiring ***underpinning methods, procedures and techniques judgment*** to create a solution within a set of ***specifically-defined conditions***."

The design or development is a logical thinking process that requires *Medical Equipment Maintainer* to apply their minds carefully in bringing solutions to specifically-defined problems. This process involves the analysis of systems or assembly of electrical and mechanical components, and integration of various elements in engineering through the application of basic and engineering sciences. Simple, straightforward calculation exercises and graphical representations from computer generated data are considered as sufficiently specifically-defined engineering design or development.

As part of demonstrating the application of theoretical knowledge, applicants must incorporate calculations with clearly defined inputs to the formulae used and detailed interpretation of the results obtained. They have to demonstrate how the calculated results have been used to provide the solution to the problem at hand, and the economic benefit to the project or the

CONTROLLED DISCLOSURE

When downloaded for the ECSA Document Management System, this document is uncontrolled and the responsibility rests with the user to ensure that it is in line with the authorised version on the database. If the 'original' stamp in red does not appear on each page, this document is uncontrolled.

Document No.: R-05-MEM-SC	Revision No.: 0	Effective Date: 09/02/2022	
Subject: Sub Discipline-specific Training Guideline for Candidate Medical Equipment Maintainers			
Compiler: MB Mtshali	Approving Officer: EL Nxumalo	Next Review Date: 09/02/2026	Page 15 of 34

operating work environment. Candidate *Medical Equipment Maintainer* must obtain experience in solving a variety of problems in their work environment, and the solution to these problems should also involve the use of fundamental engineering knowledge obtained at a university of technology or an accredited engineering institution. The problems that require scientific and engineering approach in solving them may be encountered in work required to be done on medical equipment. From their early training years, candidates must actively seek opportunities to obtain experience in the area of synthesizing solutions to real life engineering problems encountered at the workplace on medical equipment.

A suitable period of time and degree of practical participation should be sought in the workshop environment learning the basic practices that are the essence of the electrical and mechanical discipline so that the Candidate MEM's are capable of judging the efficacies of such practices in the general workplace thereafter.

7.1 Contextual Knowledge


Candidates are expected to be aware of the requirements of the engineering profession. The recognised Voluntary Association applicable to the *Medical Equipment Maintainer* and their functions and services to members, for example, provide a broad range of contextual knowledge for the Candidate *Medical Equipment Maintainer* through the full career path of the Registered *Medical Equipment Maintainer*.

The practice area of MEM's identifies specific contextual activities that are considered an essential component of the development of competence of the *Medical Equipment Maintainer*. These include awareness of basic workshop, manufacturing and fabrication activities and the competencies required of the engineer, technologist, technician, *Medical Equipment Maintainer* and artisan. Exposure to practice in these areas will be identified in each programme within the employer environment.

The Registration Assessors, Reviewers and Moderators for Specified Categories on Medical Equipment Maintainers of ECSA performs the review of the Candidate's MEM portfolio of evidence at the completion of the training period.

CONTROLLED DISCLOSURE

When downloaded for the ECSA Document Management System, this document is uncontrolled and the responsibility rests with the user to ensure that it is in line with the authorised version on the database. If the 'original' stamp in red does not appear on each page, this document is uncontrolled.

Document No.: R-05-MEM-SC	Revision No.: 0	Effective Date: 09/02/2022	
Subject: Sub Discipline-specific Training Guideline for Candidate Medical Equipment Maintainers			
Compiler: MB Mtshali	Approving Officer: EL Nxumalo	Next Review Date: 09/02/2026	Page 16 of 34

7.2 Functions Performed

Special considerations in the Medical Equipment group and each specific type of equipment or speciality must be given to the competencies specified in the following groups as described in the Degree of Responsibility scales in document **R-04-T&M-GUIDE-SC**, Table 4:

- A Knowledge based problem solving
- B Management and Communication
- C Identifying and mitigating the impacts of engineering activity
- D Judgement and responsibility
- E Independent learning

Lifting Equipment Sub Discipline-specific Requirements (Refer to Clause 8.6 below and Form R-05-SDSRR-MEM.

It is very useful to measure the progression of the candidate's competency by making use of the Degree of Responsibility scales as specified in **R-04-T&M-GUIDE-SC**, Table 4 and in clause 8.1 below.

Appendix B has been developed to align the MEM's progression with the Degree of Responsibility Scale

It should be noted that the Candidate MEM working at Responsibility level E on the Degree of Responsibility Scale carries the responsibility for work thus performed appropriate to that of a registered person except that the Candidate MEM's supervisor is accountable for the Candidates recommendations and decisions.


7.3 Industry-related statutory and other requirements

Candidates are expected to have a working knowledge of the following regulations, Acts and standards, and how they affect their working environment:

- OHS Act – Occupation Health and Safety Act, 1993 (Act No. 85 of 1993), as amended by Act No. 181 of 1993.
- National Health Act No. 63 of 2003

CONTROLLED DISCLOSURE

When downloaded for the ECSA Document Management System, this document is uncontrolled and the responsibility rests with the user to ensure that it is in line with the authorised version on the database. If the 'original' stamp in red does not appear on each page, this document is uncontrolled.

Document No.: R-05-MEM-SC	Revision No.: 0	Effective Date: 09/02/2022	
Subject: Sub Discipline-specific Training Guideline for Candidate Medical Equipment Maintainers			
Compiler: MB Mtshali	Approving Officer: EL Nxumalo	Next Review Date: 09/02/2026	Page 17 of 34

- Global Harmonisation Task Force (GHTF) document
- Environment Conservation Act, 1989 (Act No. 73 of 1989), as amended by Act No. 52 of 1994 and Act No. 50 of 2003.
- Industry specific work instructions including manufacturer instructions applicable to specific medical equipment types
- SANS and other international standards such as ISO, EN, DIN or US Federal Standards. Also refer to Appendix A.

Many other Acts not listed here may also be pertinent to a Candidate MEM's work environment. Candidate MEM's will be expected to have a basic knowledge of the applicable Acts and to investigate whether any Acts are applicable to a particular work environment.

7.4 Recommended Formal Learning Activities

The following list of formal learning is a sample of some useful course types:

- CPD courses on specific disciplines and equipment types
- Elementary Project Management
- Negotiation Skills
- Environmental Impacts
- Report writing and communication
- Planning methods
- Risk Analysis
- Quality Systems
- Occupation Health and Safety
- Maintenance Engineering

8. PROGRAMME STRUCTURE AND SEQUENCING


8.1 Best Practice

There is no ideal training programme structure or a unique sequencing that constitutes best practice.

The training programme for each Candidate MEM will depend on the work opportunities available at the time for the employer to assign to the candidate.

CONTROLLED DISCLOSURE

When downloaded for the ECSA Document Management System, this document is uncontrolled and the responsibility rests with the user to ensure that it is in line with the authorised version on the database. If the 'original' stamp in red does not appear on each page, this document is uncontrolled.

Document No.: R-05-MEM-SC	Revision No.: 0	Effective Date: 09/02/2022	
Subject: Sub Discipline-specific Training Guideline for Candidate Medical Equipment Maintainers			
Compiler: MB Mtshali	Approving Officer: EL Nxumalo	Next Review Date: 09/02/2026	Page 18 of 34

It is suggested that the Candidate MEM works with their mentors to select appropriate equipment to gain exposure to eventual responsibility for design, installation, commissioning, inspection and testing on the medical equipment selected.

The training programme should be such that Candidate MEM progresses through levels of work capability, which is described in document **R-04-T&M-GUIDE-SC**, such that by the end of the training period, the Candidate MEM must perform individually and as a team member meeting the engineering outcomes as well as the discipline-specific requirements at the level required for registration and exhibit degree of responsibility E.


The nature of work and degrees of responsibility defined in document **R-04-T&M-GUIDE-SC**, Table 4, are used here (and in **Appendix B** below):

A: Being Exposed	B: Assisting	C: Participating	D: Contributing	E: Performing
Undergoes induction, observes processes, work of competent practitioners.	Performs specific processes, under close supervision.	Performs specific processes as directed with limited supervision.	Performs specific work with detailed approval of work outputs.	Works in team without supervision, recommends work outputs, responsible but not accountable
Responsible to supervisor	Limited responsibility for work output	Full responsibility for supervised work	Full responsibility to supervisor for immediate quality of work	Level of responsibility to supervisor is appropriate to a registered person, supervisor is accountable for applicant's decisions

The Mentor and the Candidate MEM must identify at which level of responsibility an activity provides the compliance with and demonstration of the various Outcomes. The evidence of the candidate's activities will be recorded on the appropriate system such that it meets the requirements of the Training Elements, **Appendix B**. ECSA will specify the applicable recording system in the Application for Registration form (Usually an Engineering Report and a Sub-discipline Specific Requirement Report with the associated calculations, sketches, installation schedules, maintenance schedules, commission results, etcetera for each selection applied for).

CONTROLLED DISCLOSURE

When downloaded for the ECSA Document Management System, this document is uncontrolled and the responsibility rests with the user to ensure that it is in line with the authorised version on the database. If the 'original' stamp in red does not appear on each page, this document is uncontrolled.

Document No.: R-05-MEM-SC	Revision No.: 0	Effective Date: 09/02/2022	
Subject: Sub Discipline-specific Training Guideline for Candidate Medical Equipment Maintainers			
Compiler: MB Mtshali	Approving Officer: EL Nxumalo	Next Review Date: 09/02/2026	Page 19 of 34

8.2 Orientation requirements

- Introduction to Company
- Company Safety Regulations
- Company Code of Conduct
- Company Staff Code and Regulations
- Company records and record keeping
- Typical functions and activities

8.3 Realities

Generally, irrespective of the equipment type(s), it is unlikely that the period of training will be three years, the minimum time required by ECSA. Typically, it will be longer and would be determined amongst others by the availability of functions in the actual work situation.

Each candidate will effectively undertake a unique programme where the various activities carried out at the discipline-specific level are then linked to the generic competency requirements of **R-08-CS-GUIDE-SC** and the Compulsory Sub Discipline-specific Requirements to be met during the Candidacy.

8.4 Considerations for generalists, specialists, researchers and academics

Document **R-08-CS-GUIDE-SC** adequately describes what would be expected of persons whose formative development has not followed a conventional path, for example academics, researchers, specialists and those who have not followed a candidate training programme.


The overriding consideration is that, irrespective of the route followed, the applicant must provide evidence of competence against the Standard and the Sub Discipline-specific Requirements.

8.5 Moving into or Changing Candidacy Programmes

This Guide assumes that the Candidate MEM enters a programme after graduation and continues with the programme until ready to submit an application for registration. It also assumes that the Candidate MEM is supervised and mentored by persons who meet the requirements in document **R-04-T&M-GUIDE-SC**. In the case of a person changing from one

CONTROLLED DISCLOSURE

When downloaded for the ECSA Document Management System, this document is uncontrolled and the responsibility rests with the user to ensure that it is in line with the authorised version on the database. If the 'original' stamp in red does not appear on each page, this document is uncontrolled.

Document No.: R-05-MEM-SC	Revision No.: 0	Effective Date: 09/02/2022	
Subject: Sub Discipline-specific Training Guideline for Candidate Medical Equipment Maintainers			
Compiler: MB Mtshali	Approving Officer: EL Nxumalo	Next Review Date: 09/02/2026	Page 20 of 34

candidacy programme to another or moving into a candidacy programme from a less structured environment, it is essential that the following steps be completed:

- The Candidate MEM must complete the Training and Experience Summary (TES) and Training and Experience Reports (TER) for the previous programme or unstructured experience. In the latter case it is important to reconstruct the experience as accurately as possible. The TERs must be signed off.
- On entering the new programme, the Mentor and Supervisor should review the Candidate MEM's development in the light of the past experience and opportunities and requirements of the new programme and plan at least the next phase of the candidate's programme.
- The Candidate MEM must complete the Sub Discipline-specific Requirements Report (SDSRR) on elements already covered during the first part of the candidacy.

8.6 Compulsory Sub Discipline-specific Requirements to be met during the Candidacy

There is a critical need in the industry to identify people who are able to conduct the essential operations associated with efficient and safe medical equipment design, installation, commissioning, maintenance and inspection. This will lead to competence in the field of work and thereby add value to the industry and improve the economy of the country. It will also lead to a balanced society in that learners will understand how the work they do fits into the greater engineering industry.


The Candidate assisted by Mentors and Supervisors must during candidacy ensure that he or she is conversant with the practical knowledge set out in the forms listed below, and submit evidence as such as part of the Application for Registration form.

Applications for a specified category practitioner in medical equipment design, installation, commissioning, maintenance and inspection must submit the Sub Discipline-specific Requirements Report (SDSRR) form **R-05-SDSRR-MEM** below.

This form is part of the applicable Application for Registration Forms.

CONTROLLED DISCLOSURE


When downloaded for the ECSA Document Management System, this document is uncontrolled and the responsibility rests with the user to ensure that it is in line with the authorised version on the database. If the 'original' stamp in red does not appear on each page, this document is uncontrolled.

Document No.: R-05-MEM-SC	Revision No.: 0	Effective Date: 09/02/2022	
Subject: Sub Discipline-specific Training Guideline for Candidate Medical Equipment Maintainers			
Compiler: MB Mtshali	Approving Officer: EL Nxumalo	Next Review Date: 09/02/2026	Page 21 of 34

The Candidate assisted by Mentors and Supervisors must during candidacy ensure that he or she is conversant with the practical knowledge set out in form R-05-SDSRR-MEM, and submit evidence as such.

CONTROLLED DISCLOSURE

When downloaded for the ECSA Document Management System, this document is uncontrolled and the responsibility rests with the user to ensure that it is in line with the authorised version on the database. If the 'original' stamp in red does not appear on each page, this document is uncontrolled.

Document No.: R-05-MEM-SC	Revision No.: 0	Effective Date: 09/02/2022	
Subject: Sub Discipline-specific Training Guideline for Candidate Medical Equipment Maintainers			
Compiler: MB Mtshali	Approving Officer: EL Nxumalo	Next Review Date: 09/02/2026	Page 22 of 34


REVISION HISTORY

Revision number	Revision date	Revision details	Approved by
Concept A	3 July 2013	Initial attempt at LMI DSTG based on R-05-MEC-PN with own Annexures A and B added. Needs input from MEM Registration Committee and CRC Specified Category Working Group	CRC Working Group
Concept B	19 December 2018	Revised to align with Fire Protection System Practitioner concept document R-05-FPSP-SC. Needs final input from MEM Steering Committee	CRC Working Group
Rev. 0 Draft A	31 August 2021	Reviewed as per the four-year review cycle and aligned to the Discipline-Specific Guide Framework.	Alignment by RPS:BU
Rev. 0 Draft B	28 September 2021	Alignment to the Discipline-Specific Guide Framework.	Executive: RPS – EL Nxumalo
Rev. 0	09 February 2022	Approval	RPSC

The Discipline-specific Training Guide for:

Candidate Medical Equipment Maintainers

Revision 0 dated 09 February 2022 and consisting of 22 pages has been reviewed for adequacy by the Business Unit Manager and is approved by the Executive: Research Policy and Standards (RPS).



 Business Unit Manager

..09/03/2022.....
 Date




 Executive: RPS

..2022/03/09.....
 Date

This definitive version of this policy is available on our website.

CONTROLLED DISCLOSURE

When downloaded for the ECSA Document Management System, this document is uncontrolled and the responsibility rests with the user to ensure that it is in line with the authorised version on the database. If the 'original' stamp in red does not appear on each page, this document is uncontrolled.

Document No.: R-05-MEM-SC	Revision No.: 0	Effective Date: 09/02/2022	
Subject: Sub Discipline-specific Training Guideline for Candidate Medical Equipment Maintainers			
Compiler: MB Mtshali	Approving Officer: EL Nxumalo	Next Review Date: 09/02/2026	Page 23 of 34

Sub Discipline-Specific Requirements Report

Form R-05-SDSRR-MEM


Surname and Initials:

Use this form to report in not more than 100 words per statement under Requirements 1 to 6 below on the applicant's personal knowledge about the requirements. Attach to this report the actual work schedule and load test report for each equipment type (listed on page 1 of the Engineering Report, Form R-03-ER-SC) applied for, done by the applicant under the supervision of a registered MEM (Medical Equipment Maintainer).

<u>SUB DISCIPLINE-SPECIFIC KNOWLEDGE REQUIREMENTS:</u>	
1.	
Apply problem solving skills to maintain medical equipment	
1.1 Describe the operation of machines in terms of the processes of enhancing human performance.	
1.2 Identify variances from medical equipment specifications in a methodical manner that includes all areas of performance.	
1.3 Follow logical procedures to correct all identified variances.	
1.4 Correct variances in accordance with recognised clinical engineering procedures or codes of practice.	
1.5 Identify alternative solutions to problems that will provide similar results.	
2.	
Maintain medical equipment	
2.1 Understand the application and operation of medical equipment in the clinical environment. Describe the operation of any <u>one</u> medical apparatus.	
2.2 Source and confirm the policies for maintenance work for applicability with relevant sources.	
2.3 Prepare the work area for the relevant activities in accordance with workplace requirements.	
2.4 State how you Identified defects from user reports and test procedures?	
2.5 Use tools and test equipment appropriate to the type of medical equipment. What typical test equipment would you use on what type medical apparatus?	
2.6 Identify faults through logical fault finding procedures. Explain any one procedure!	

CONTROLLED DISCLOSURE


When downloaded for the ECSA Document Management System, this document is uncontrolled and the responsibility rests with the user to ensure that it is in line with the authorised version on the database. If the 'original' stamp in red does not appear on each page, this document is uncontrolled.

Document No.: R-05-MEM-SC	Revision No.: 0	Effective Date: 09/02/2022	
Subject: Sub Discipline-specific Training Guideline for Candidate Medical Equipment Maintainers			
Compiler: MB Mtshali	Approving Officer: EL Nxumalo	Next Review Date: 09/02/2026	Page 24 of 34

2.7 Repair, maintain and calibrate medical equipment in accordance with manufacturer specifications and relevant policies. Where did you obtain the specifications and how did you go about it?	
2.8 How did you check equipment performance and safety inspections according to the relevant check lists and specifications before returning equipment to use	
2.9 Capture and record accurate equipment history for future reference for a time period relevant to equipment type maintained and legal policies. How did you obtain this?	
3. Apply scientific and engineering skills to maintain medical equipment	
3.1 Explain work functions required in maintaining medical equipment in terms of quality in engineering practice.	
3.2 Identify engineering risks in terms of potential impact for each risk on safety and performance of medical equipment.	
3.3 Analyse actions to improve work functions in terms of available options.	
3.4 Explain fabrication principles for fabrication of required components in terms of functions and accuracy. Describe one example?	
3.5 Test and repair electrical circuits in accordance with manufacturer specifications.	
3.6 Explain flow characteristics in terms of engineering principles related to medical equipment to be maintained. Describe one example to illustrate this?	
4. Communicate maintenance information for medical equipment	
4.1 Generate maintenance reports from relevant data in accordance with workplace procedures. Explain how you go about it!	
4.2 Communicate clear, unambiguously and at an appropriate level for designated target audiences. What information, to who and at what level do you report?	
5. Comply with relevant legislation in maintaining medical equipment	
5.1 Obtain authorisation to conduct activities in accordance with workplace procedures.	
5.2 Identify and report potential hazardous conditions in accordance with workplace requirements.	
5.3 Identify and report deviances from acceptable standards to the relevant stakeholder in accordance with statutory requirements and manufacturer specifications.	
5.4	

CONTROLLED DISCLOSURE


When downloaded for the ECSA Document Management System, this document is uncontrolled and the responsibility rests with the user to ensure that it is in line with the authorised version on the database. If the 'original' stamp in red does not appear on each page, this document is uncontrolled.

Document No.: R-05-MEM-SC	Revision No.: 0	Effective Date: 09/02/2022	
Subject: Sub Discipline-specific Training Guideline for Candidate Medical Equipment Maintainers			
Compiler: MB Mtshali	Approving Officer: EL Nxumalo	Next Review Date: 09/02/2026	Page 25 of 34

Explain the consequences of omitting procedures in terms of potential risks and liability.	
5.5 Complete maintenance activities within agreed timeframes. Explain the importance of completing activities in these timeframes in terms of customer service and work interruptions.	
6. Comply with accepted work ethics and good practice when maintaining medical equipment	
6.1 Explain the code of conduct in accordance with relevant acts, and practice as it relates to maintaining medical equipment. Write down the principles of the code?	

CONTROLLED DISCLOSURE

When downloaded for the ECSA Document Management System, this document is uncontrolled and the responsibility rests with the user to ensure that it is in line with the authorised version on the database. If the 'original' stamp in red does not appear on each page, this document is uncontrolled.

Document No.: R-05-MEM-SC	Revision No.: 0	Effective Date: 09/02/2022	
Subject: Sub Discipline-specific Training Guideline for Candidate Medical Equipment Maintainers			
Compiler: MB Mtshali	Approving Officer: EL Nxumalo	Next Review Date: 09/02/2026	Page 26 of 34


APPENDIX A:

SPECIFIC EQUIPMENT TYPES RECOGNISED FOR REGISTRATION AS A MEDICAL EQUIPMENT TECHNICIAN

<u>No.</u>	<u>Description of Equipment Type</u>	<u>Standard Applicable (Indicate as appropriate)</u>
1.	Mechanical Equipment	
2.	Electro-medical equipment	
3.	Respiratory and anaesthetic equipment	
4.	Medical imaging equipment	

CONTROLLED DISCLOSURE

When downloaded for the ECSA Document Management System, this document is uncontrolled and the responsibility rests with the user to ensure that it is in line with the authorised version on the database. If the 'original' stamp in red does not appear on each page, this document is uncontrolled.

Document No.: R-05-MEM-SC	Revision No.: 0	Effective Date: 09/02/2022	
Subject: Sub Discipline-specific Training Guideline for Candidate Medical Equipment Maintainers			
Compiler: MB Mtshali	Approving Officer: EL Nxumalo	Next Review Date: 09/02/2026	Page 27 of 34

Training Elements

This guide is written for the recent graduate who is training and gaining experience toward registration (“Benchmark Route”). Mature applicants for registration (“Alternative Route”) may apply the guide retrospectively to identify possible gaps in their development

Synopsis: A candidate specified category practitioner should achieve specific competencies at the prescribed level during his/her development towards registration, at the same time accepting more and more responsibility as experience is gained. The outcomes achieved and established during the candidacy phase should form the template to all engineering work performed after registration, regardless of the level of responsibility at any particular stage of an engineering career:


1. Confirm understanding of instructions received and clarify if necessary;
2. Use theoretical training to develop possible approaches to do the work: select the best and present to the recipient;
3. Apply theoretical knowledge to justify decisions taken and processes used;
4. Understand role in the work team, and plan and schedule work accordingly;
5. Issue complete and clear instructions and report comprehensively on work completed;
6. Be sensitive about the impact of the engineering activity and take action to mitigate this impact;
7. Consider and adhere to legislation applicable to the task and the associated risk identification and management;
8. Adhere strictly to high ethical behavioural standards and ECSA’s Code of Conduct;
9. Display sound judgement by considering all factors, their interrelationship, consequences, and evaluation when all evidence is not available;
10. Accept responsibility for own work by using theory to support decisions, seeking advice when uncertain, and evaluating shortcomings; and
11. Become conversant with employer’s training and development program and develop own lifelong development program within this framework.

Specifically-defined engineering work is usually restricted to applying standard procedures, codes and systems, i.e. work that was done before within the narrow field of application.

Responsibility Levels: A = Being Exposed; B = Assisting; C = Participating; D = Contributing; E = Performing.

CONTROLLED DISCLOSURE


When downloaded for the ECSA Document Management System, this document is uncontrolled and the responsibility rests with the user to ensure that it is in line with the authorised version on the database. If the 'original' stamp in red does not appear on each page, this document is uncontrolled.

Document No.: R-05-MEM-SC	Revision No.: 0	Effective Date: 09/02/2022	
Subject: Sub Discipline-specific Training Guideline for Candidate Medical Equipment Maintainers			
Compiler: MB Mtshali	Approving Officer: EL Nxumalo	Next Review Date: 09/02/2026	Page 28 of 34

Competency Standards for Registration as a Specified Category Practitioner	Explanation and Responsibility Level
<p>1. Purpose This standard defines the competence required for registration as a Specified Category Practitioner. Definitions of terms having particular meaning within this standard are given in text at the end of this Annexure and in document R-01-POL-SC.</p>	<p>Discipline Specific Training Guides (DSTG) gives context to the purpose of the Competency Standards. Registered Specified Category Practitioner operate within the nine disciplines recognised by ECSA. Each discipline can be further divided into sub-disciplines and finally into specific workplaces or competency areas <u>DSTG's are used to facilitate experiential development towards ECSA registration and assist in compiling the required portfolio of evidence (Specifically the Engineering Report in the application form).</u> NOTE: The training period must be utilised to develop the competence of the trainee towards achieving the standards below at a responsibility as indicated (mostly level E, i.e. Performing. Refer to R-04-T&M-GUIDE-SC, Table 4)</p>
<p>2. Demonstration of Competence Competence must be demonstrated within specifically-defined engineering activities, defined below, by integrated performance of the outcomes defined in section 3 below at the level defined for each outcome. Required contexts and functions may be specified in the applicable Sub-discipline Specific Training Requirements. Level Descriptor: <u>Specifically-defined engineering activities</u> have several of the following characteristics:</p> <ol style="list-style-type: none"> Scope of specific practice area is defined by specific techniques applied; change by adopting new specific techniques into current practice; Practice area is located within a wider, complex <i>context</i>, with specifically-defined working relationships with other parties and disciplines; Work involves specific familiar <i>resources</i>, including people, money, equipment, materials, technologies; Require resolution of <i>interactions</i> manifested between specific technical factors with limited impact on wider issues; Are <i>constrained</i> by operational context, defined work package, time, finance, infrastructure, resources, facilities, standards and codes, applicable laws; Have <i>risks</i> and <i>consequences</i> that are locally important but are specifically defined. <p>Activities include but are not limited to: planning; investigation and problem resolution; improvement of materials, components, systems or processes, engineering operations, maintenance, project management, development and commercialisation.</p>	<p>Engineering activities can be divided into (approximately): 5% Complex (Professional Engineers) 5% Broadly Defined (Professional Engineering Technologists) 10% Well-defined (Professional Engineering Technicians) 15% Specifically-defined (Registered Specified Categories) 20% Skilled Workman (Engineering Artisan) 45% Unskilled Workman (Artisan Assistants)</p> <p>The activities can be in-house or contracted out; evidence of integrated performance can be submitted irrespective of the situation. Level Descriptor: <u>Specifically-defined engineering activities</u> in the specific discipline is characterised by several or all of:</p> <ol style="list-style-type: none"> Scope of practice area does not cover the entire field of the specific discipline (exposure limited to the relevant components of the specific sub-discipline and specific workplace). Techniques applied are largely well established and change by adopting new specific techniques into current practice is the exception; Practice area varies substantially with unlimited location possibilities and an additional responsibility to identify the need for <i>complex, broadly defined and/or well-defined</i> advice to be included in the specifically-defined working relationships with other parties and disciplines; The bulk of the work involves familiar, defined range of <i>resources</i>, including people, money, equipment, materials, technologies; Most of the impacts in the specific discipline are on wider issues, and although occurring frequently, are <i>specifically-defined</i> and can be resolved by following established procedures. The work packages and associated parameters are <i>constrained</i> by operational context with variations limited to different locations only. (Cannot be covered by laws, standards and codes only). Even locally important minor risks can have far reaching consequences. <p>Activities include but are not limited to: design; planning; investigation and problem resolution; improvement of materials, components, systems or processes; engineering operations; maintenance; project management and general management. For Specified Category Practitioners, research, development and commercialisation happen more frequently in some disciplines and are seldom encountered in others.</p>

CONTROLLED DISCLOSURE


When downloaded for the ECSA Document Management System, this document is uncontrolled and the responsibility rests with the user to ensure that it is in line with the authorised version on the database. If the 'original' stamp in red does not appear on each page, this document is uncontrolled.

Document No.: R-05-MEM-SC	Revision No.: 0	Effective Date: 09/02/2022	
Subject: Sub Discipline-specific Training Guideline for Candidate Medical Equipment Maintainers			
Compiler: MB Mtshali	Approving Officer: EL Nxumalo	Next Review Date: 09/02/2026	Page 29 of 34

3. Outcomes to be satisfied:	Explanation and Responsibility Level
Group A: Engineering Problem Solving.	
Outcome 1: Define, investigate and analyse specifically-defined engineering problems (tasks)	Responsibility level E Analysis of an engineering problem means the “separation into parts possibly with comment and judgement”.
Level Descriptor: <i>Specifically-defined engineering <u>problems</u> have the following characteristics:</i> (a) can be solved mainly by specific practical engineering knowledge, underpinned by related theory; and one or more of: (b) are fully defined but require feedback; (c) are discrete, specifically focused tasks within engineering systems; (d) are routine, frequently encountered and in familiar specified context; and one or more of: (e) can be solved by standardized or prescribed ways; (f) are encompassed by specific standards, codes and documented procedures; requires authorization to work outside limits; (g) information is concrete, specific and largely complete, but requires checking and possible supplementation; (h) involve specific issues but few of these imposing conflicting constraints and a specific range of interested and affected parties; and one or both of: (i) requires practical judgement in specific practice area in evaluating solutions, considering interfaces to other role-players; (j) have consequences which are locally important but within a specified category (wider impact are dealt with by others).	(a) practical problems for Specified Category Practitioners means the problem encountered cannot be solved by artisans because theoretical calculations and engineering decisions are necessary to substantiate the solution proposed; (b) further investigation to identify the nature of the problem is seldom necessary; (c) discrete means <i>individually distinct</i> . The problem is easily recognised as part of the larger engineering task, project or operation; (d) recognised that the problem is within the specific scope and occurred in the past, or the work to be done is a standard operation – seldom something new; (e) solving the problem does not require the development of a new solution – find out how it was solved/done before; (f) encompassed means <i>encircled</i> : The standards, codes and documented procedures must be obtained to solve the problem and ; authorisation from Professionals responsible must be obtained to waive the stipulations; (g) the responsibility lies with the Specified Category Practitioner to check that the information received as part of the instruction is correct, and added to as is necessary to ensure the correct and complete execution of the work; (h) the problem handled by an Specified Category Practitioner must be limited to well know specific matters needing standardised solutions without possible complications; (i) practical solutions to problems include knowledge of the skills displayed by Practical Specialists and Engineering Artisans without sacrificing theoretical engineering principles and / or cutting corners to satisfy parties involved; (j) Specified Category Practitioners must realise that their engineering actions might seem to be of local importance only, but may develop into further problems where support from Engineering Professionals might be needed to deal with these consequences.
Competency Indicators: A structured analysis of specifically-defined problems typified by the following performances within the competency area is expected: 1.1 State how <u>you</u> interpreted the work instruction received, checking with your client or supervisor if your interpretation is correct 1.2 Describe how <u>you</u> analysed, obtained and evaluated further clarifying information, and if the instruction was revised as a result.	To perform an engineering task a Specified Category Practitioner will typically receive an instruction from a senior person (customer) to do this task, and must: 1.1 Make very sure that the instruction is complete, clear and within his/her capability and that the person who issued the instruction agrees with his/her interpretation. 1.2 Ensure that the instruction and information to do the work is fully understood and is complete, including the engineering theory needed to understand the task and to carry out and/or check calculations, and the acceptance criteria. If needed supplementary information must be gathered, studied and understood.
Range Statement: The problem (task) may be part of a larger engineering activity or may be stand alone. The design (plan-ning) problem is amenable to solution by specific techniques practiced regularly. This outcome is concerned with the under-standing of a problem: Outcome 2 is concerned with the solution.	Please refer to clauses 5 to 8 of the applicable Sub-discipline Specific Training Guide, document R-05-MEM-SC

CONTROLLED DISCLOSURE


When downloaded for the ECSA Document Management System, this document is uncontrolled and the responsibility rests with the user to ensure that it is in line with the authorised version on the database. If the 'original' stamp in red does not appear on each page, this document is uncontrolled.

Document No.: R-05-MEM-SC	Revision No.: 0	Effective Date: 09/02/2022	
Subject: Sub Discipline-specific Training Guideline for Candidate Medical Equipment Maintainers			
Compiler: MB Mtshali	Approving Officer: EL Nxumalo	Next Review Date: 09/02/2026	Page 30 of 34

<p>Outcome 2: Design or develop (plan) sustainable solutions to specifically-defined engineering problems (tasks).</p> <p>Competency Indicators: This outcome is normally demonstrated after a problem analysis as defined in outcome 1. Working systematically to synthesise a solution to a well-defined problem, typified by the following performances is expected:</p> <p>2.1 Describe how <u>you</u> designed or developed and analysed alternative approaches to do the work. Impacts and sustainability checked. Calculations attached</p> <p>2.2 State what the final solution to perform the work was, client or your supervisor in agreement</p>	<p>Responsibility level C Design means “drawing or outline from which something can be made”. Develop means “come or bring into a state in which it is active or visible”.</p> <p>The task given must be fully understood and interpreted; solutions developed (designed) to execute. To synthesise a solution means “the combination of separate parts, elements, substances, etc. into a whole or into a system” by:</p> <p>2.1 The development (design) of more than one way to do an engineering task or solve a problem should always be done, including the costing and impact assessment for each alternative. All the alternatives must meet the requirements set out by the instruction received, and <u>the theoretical calculations to support each alternative must be done and submitted as an attachment</u>. The alternatives must be within the legal boundaries imposed.</p> <p>2.2 The Specified Category Practitioner will in some cases not be able to support proposals with the complete theoretical calculation to substantiate every aspect, and must in these cases refer his / her alternatives to a Professional for scrutiny and support. The alternatives and alternative recommended must be convincingly detailed to win customer support for the alternative recommended. Selection of alternatives might be based on tenders submitted with alternatives submitted deviating from those specified.</p>
<p>Range Statement: The solution conforms to specific established methods, techniques or procedures within the specifically-defined competency area. Engineering should not look only to decrease impacts, but also to restore and regenerate through design.</p>	<p>Applying theory to <i>specifically-defined engineering</i> work is done in a way that’s been used before, probably developed by Professionals in the past, and documented in written procedures, specifications, drawings, models, examples, etc. Specified Category Practitioners must seek approval and engineering verification for any deviation from these established methods.</p>
<p>Outcome 3: Comprehend and apply knowledge embodied in established specific engineering practices and knowledge specific to the field in which he/she practices.</p> <p>Competency Indicators: This outcome is normally demonstrated in the course of design, investigation or operations, confined to the competency area.</p> <p>3.1 State what HCert level <u>engineering standard procedures and systems you</u> used to execute the work, and how HCert level theory was applied to understand and/or verify these procedures;</p> <p>3.2 Give <u>your</u> own HCert level theoretical calculations and/or reasoning on why the application of this theory is considered to be correct (Actual examples).</p>	<p>Responsibility level E Comprehend means “to understand fully”. The jurisdiction in which a Specified Category Practitioner practices is given in Clauses 5 to 8 of the applicable Discipline Specific Training Guide, document R-05-nnn-SC</p> <p>Design (development) work for Specified Category Practitioners is mostly to utilise, configure, certify, test, verify, etc. manufactured components or proven engineering or management systems, and repetitive design (development) work using an existing design (development) as an example. Specified Category Practitioners apply existing codes, policies and procedures in their design (development) work. Investigations on specifically-defined incidents and condition monitoring and operations mostly on controlling, maintaining and improving engineering systems and operations.</p> <p>3.1 The understanding of specifically-defined procedures and techniques must be based on fundamental mathematical, scientific and engineering knowledge. Specific procedures and techniques applied to do the work accompanied by the underpinning theory must be given.</p> <p>3.2 Calculations confirming the correct application and utilisation of equipment and/or systems listed in the Sub-discipline Specific Training Guide R-05-nnn-SC must be done on practical <i>specifically-defined</i> activities. Reference must be made to standards and procedures used and how it was derived from HCert level theory.</p>
<p>Range Statement: Applicable knowledge includes:</p> <p>(a) Technical knowledge that is applicable to the practice area irrespective of location, supplemented by locally relevant knowledge, for example established properties of local materials.</p> <p>(b) A working knowledge of interacting disciplines confined to the</p>	<p>(a) The specific location of a task to be executed is the most important determining factor in the layout design and utilisation of equipment and/or systems. A combination of educational knowledge and practical experience must be used to substantiate decisions taken including a comprehensive study of laws, policies, procedures, standards, environment, manpower, materials, components and projected customer requirements and expectations.</p>

CONTROLLED DISCLOSURE

When downloaded for the ECSA Document Management System, this document is uncontrolled and the responsibility rests with the user to ensure that it is in line with the authorised version on the database. If the 'original' stamp in red does not appear on each page, this document is uncontrolled.


Document No.: R-05-MEM-SC	Revision No.: 0	Effective Date: 09/02/2022	
Subject: Sub Discipline-specific Training Guideline for Candidate Medical Equipment Maintainers			
Compiler: MB Mtshali	Approving Officer: EL Nxumalo	Next Review Date: 09/02/2026	Page 31 of 34

<p>competency area. Codified knowledge in related areas: financial, statutory, safety, management and sustainability.</p> <p>(c) Jurisdictional knowledge includes legal and regulatory requirements as well as prescribed codes of practice.</p>	<p>(b) In spite of having a working knowledge of interacting disciplines, Specified Category Practitioners must appreciate the importance of working with specialists like Civil Engineers on structures and roads, Mechanical Engineers on fire protection equipment, Architects on buildings, Electrical Engineers on communication equipment, etc. The codified knowledge in the related areas means working to and understanding the requirements set out by specialists in the areas mentioned.</p> <p>(c) Jurisdictional in this instance means “having the authority”, and Specified Category Practitioners must adhere to the terms and conditions associated with each task undertaken. They may even be appointed as the “responsible person” for specific duties in terms of the OHS Act.</p>
---	--

Group B: Managing Engineering Activities.	Explanation and Responsibility Level
<p>Outcome 4: Manage part or all of one or more <i>specifically-defined</i> engineering activities.</p> <p>Competency Indicators: The display of personal and work process management abilities within the competency area is expected: 4.1 State how <u>you</u> managed yourself, priorities, processes and resources in doing the work (e.g. bar chart); 4.2 Describe <u>your</u> role and contribution in the work team.</p>	<p>Responsibility level E Manage means “control”.</p> <p>In engineering operations and projects Specified Category Practitioners will typically be given the responsibility to carry out specific tasks and/or complete projects. 4.1 Resources are usually subdivided based on availability and controlled by a work breakdown structure and scheduling to meet deadlines. Quality, safety and environment management are important aspects. 4.2 Depending on the task, Specified Category Practitioners can be the manager, team leader, a team member, or can supervise appointed contractors.</p>
<p>Outcome 5: Communicate clearly with others in the course of his or her specifically-defined engineering activities</p> <p>Competency Indicators: Demonstrates effective communication by: 5.1 State how <u>you</u> presented your point of view and compiled reports after completion of the work. 5.2 State how <u>you</u> compiled and issued instructions to entities working on the same task</p>	<p>Responsibility level E</p> <p>5.1 Refer to Range State for Outcome 4 and 5 below. Presentation of point of view mostly occurs in meetings and discussions with immediate supervisor. 5.2 Refer to Range State for Outcome 4 and 5 below.</p>
<p>Range Statement for Outcomes 4 and 5: Management and communication in <i>specifically-defined engineering</i> involves: (a) Planning activities; (b) Organising activities; (c) Leading activities; (d) Implementing activities, and (e) Controlling activities. Communication relates to technical aspects and wider impacts of professional work. Audience includes peers, other disciplines, clients and stakeholders audiences. Appropriate modes of communication must be selected. The Specified Category Practitioner is expected to perform the communication functions reliably and repeatedly confined to the competency area,</p>	<p>(a) Planning means “the arrangement for doing or using something, considered in advance”. (b) Organising means “put into working order; arrange in a system; make preparations for”. (c) Leading means to “guide the actions and opinions of; influence; persuade”. (d) Implementing means to “carry an undertaking, agreement, or promise into effect”. (e) Controlling means the “means of regulating, restraining, keeping in order; check”. Specified Category Practitioners participate in writing or adhere to specifications for the purchase of materials and/or work to be done, recommendation on tenders received, place orders and variation orders, write work instructions, report back on work done, draw, correct and revise drawings, compile test reports, use operation and maintenance manuals to write or apply work procedures, write inspection and audit reports, write commissioning reports, prepare and present motivations for new projects, compile budgets, report on studies done and calculations carried out, report on customer requirements, report on safety incidents and risk analysis, report on equipment failure, report on proposed system improvement and new techniques, report back on cost control, report on environmental impact and sustainability, etc.</p>

CONTROLLED DISCLOSURE


When downloaded for the ECSA Document Management System, this document is uncontrolled and the responsibility rests with the user to ensure that it is in line with the authorised version on the database. If the 'original' stamp in red does not appear on each page, this document is uncontrolled.

Document No.: R-05-MEM-SC	Revision No.: 0	Effective Date: 09/02/2022	
Subject: Sub Discipline-specific Training Guideline for Candidate Medical Equipment Maintainers			
Compiler: MB Mtshali	Approving Officer: EL Nxumalo	Next Review Date: 09/02/2026	Page 32 of 34

Group C: Impacts of Engineering Activity.	Explanation and Responsibility Level
Outcome 6: Recognise the foreseeable social, cultural, environmental and sustainability effects of <i>specifically-defined</i> engineering activities generally	Responsibility level D Social means "people living in communities; of relations between persons and communities". Cultural means "all the arts, beliefs, social institutions, etc. characteristic of a community". Environmental means "surroundings, circumstances, influences". Sustainable is defined in the definitions below.
Competency Indicators: This outcome is normally displayed in the course of analysis and solution of problems within the competency area, by typically: 6.1 Describe the social, cultural, environmental impact and long term sustainability of this engineering activity; 6.2 State how <u>you</u> communicated mitigating measures to affected parties and acquired stakeholder engagement.	6.1 Engineering impacts heavily on the environment e.g. servitudes, expropriation of land, excavation of trenches with associated inconvenience, borrow pits, dust and obstruction, street and other crossings, power dips and interruptions, visual and noise pollution, malfunctions, oil and other leaks, electrocution of human beings, detrimental effect on animals and wild life, dangerous rotating and other machines, demolishing of structures, etc. 6.2 Mitigating measures taken may include environmental impact studies, environmental impact management, community involvement and communication, barricading and warning signs, temporary crossings, alternative supplies (ring feeders and bypass roads), press releases, compensation paid, etc.
Outcome 7: Meet all legal and regulatory requirements, protect the health and safety of persons and adhere to sustainable practices in the course of his or her specifically-defined engineering activities.	Responsibility level E
Competency Indicators: 7.1 List the major laws and regulations applicable to this particular activity and how sustainability practices and health and safety matters were handled; 7.2 State how <u>you</u> obtained advice in doing risk management for the work and elaborate on the risk management system applied.	7.1 The OHS Act is supplemented by a variety of parliamentary acts, regulations, local authority by-laws, standards and codes of practice. Places of work might have standard procedures, instructions, drawings and operation and maintenance manuals available. These documents, depending on the situation (emergency, breakdown, etc.) are consulted before work is commenced and during the activity; 7.2 It is advisable to attend a Risk Management (Assessment) course, and to investigate and study the materials, components and systems used in the workplace. The Specified Category Practitioners seeks advice from knowledgeable and experienced specialists if any doubt exist that safety and sustainability cannot be guaranteed.
Range Statement for Outcomes 6 and 7: Impacts and regulatory requirements include: (a) Impacts to be considered are generally those identified within the established methods, techniques or procedures used in the specific practice area; (b) Regulatory requirements are prescribed; (c) Apply prescribed risk management strategies; (d) Effects to be considered and methods used are defined; (e) Prescribed safe and sustainable materials, components and systems. (f) Prescribe maintenance protocols; (g) Persons whose health and safety are to be protected are both inside and outside the workplace.	(a) The impacts will vary substantially with the location of the task, e.g. the impact of laying a cable or pipe in the main street of town will be entirely different to construction in a rural area. The methods, techniques or procedures will differ accordingly, and is identified and studied by the Specified Category Practitioners before starting the work. (b) The Safety Officer and/or the Responsible Person appointed in accordance with the OHS Act usually confirm or check that the instructions are in line with regulations. The Specified Category Practitioners is responsible to see to it that this is done, and if not, establishes which regulations apply, and ensure that they are adhered to. Usually the people working on site are strictly controlled w.r.t. health and safety, but the Specified Category Practitioners checks that this is done. Tasks and projects are mostly carried out where contact with the public cannot be avoided, and safety measures like barricading and warning signs must be used and maintained. (c) Risks are mostly associated with elevated structures, subsidence of soil, electrocution of human beings, moving parts on machinery, fraud and corruption and theft. Risk management strategies are usually done by

CONTROLLED DISCLOSURE

When downloaded for the ECSA Document Management System, this document is uncontrolled and the responsibility rests with the user to ensure that it is in line with the authorised version on the database. If the 'original' stamp in red does not appear on each page, this document is uncontrolled.


Document No.: R-05-MEM-SC	Revision No.: 0	Effective Date: 09/02/2022	
Subject: Sub Discipline-specific Training Guideline for Candidate Medical Equipment Maintainers			
Compiler: MB Mtshali	Approving Officer: EL Nxumalo	Next Review Date: 09/02/2026	Page 33 of 34

	<p>more senior staff, but are understood and applied by the Specified Category Practitioners.</p> <p>(d) Effects associated with risk management are mostly well known if not obvious, and methods used to address, clearly defined.</p> <p>(e) Usually the safe and sustainable materials, components and systems are prescribed by Professionals or other specialists. It is the responsibility of the Specified Category Practitioners to use his/her knowledge and experience to check and interpret what is prescribed and report anything that he/she is not satisfied with.</p> <p>(f) Draw up maintenance systems and procedures from Codes of Practice and Manufacturer's Instructions.</p> <p>(g) Staff working on the task or project as well as persons affected by the engineering work being carried out.</p>
--	---

Group D: Exercise judgment, take responsibility, and act ethically.	Explanation and Responsibility Level
Outcome 8: Conduct engineering activities ethically.	Responsibility level E Ethically means "science of morals; moral soundness". Moral means "moral habits; standards of behaviour; principles of right and wrong".
Competency Indicators: Sensitivity to ethical issues and the adoption of a systematic approach to resolving these issues is expected, typified by: 8.1 State how <u>you</u> identified ethical issues and affected parties and their interest and what you did about it when a problem arose. 8.2 Confirm that <u>you</u> are conversant and in compliance with ECSA's Code of Conduct and why this is important in your work.	Systematic means "methodical; based on a system". 8.1 Ethical problems that can occur include tender fraud, payment bribery, alcohol abuse, sexual harassment, absenteeism, favouritism, defamation, fraudulent overtime claims, fraudulent expenses claimed, fraudulent qualifications, misrepresentation of facts, etc. 8.2 ECSA's Code of Conduct, as per ECSA's website, is known and adhered to. Applicable examples given.
Outcome 9: Exercise sound judgement in the course of <i>specifically-defined</i> engineering activities	Responsibility level E Judgement means "good sense: ability to judge".
Competency Indicators: Exhibition of judgement is expected by: 9.1 State the factors applicable to the work, their interrelationship and how <u>you</u> applied the most important factors; 9.2 Describe how <u>you</u> foresaw work consequences and evaluated situations in the absence of full evidence.	9.1 The extent of a project or task given to a junior Specified Category Practitioner is characterised by the limited number of factors and their resulting interdependence. He/she will seek advice if educational and/or experiential limitations are exceeded. Examples of the main engineering factors applied must be given. 9.2 Taking risky decisions will lead to equipment failure, excessive installation and maintenance cost, damage to persons and property, bankruptcy, poor service delivery, etc. Give examples.
Range Statement for Outcomes 8 and 9: Judgement is expected both within the application of the candidate's category specific methods, techniques and specific procedures and in assessing their immediate impacts. Judgement in decision making involves: (a) taking limited risk factors into account some of which may be ill-defined; or (b) consequences are in the immediate work contexts; or (c) identified set of interested and affected parties with defined needs to be taken into account.	In engineering about 15% of the activities can be classified as <i>specifically-defined</i> where the Specified Category Practitioner uses standard procedures, codes of practice, specifications, etc. Judgement must be displayed to identify any activity falling outside the <i>specifically-defined</i> range, as defined above by: (a) Seeking advice when risk factors exceed his/her capability. (b) Consequences outside the immediate work contexts, e.g. long-term, not normally handled. (c) Interested and affected parties with defined needs outside the <i>specifically-defined</i> parameters to be taken into account.

CONTROLLED DISCLOSURE

When downloaded for the ECSA Document Management System, this document is uncontrolled and the responsibility rests with the user to ensure that it is in line with the authorised version on the database. If the 'original' stamp in red does not appear on each page, this document is uncontrolled.

Document No.: R-05-MEM-SC	Revision No.: 0	Effective Date: 09/02/2022	
Subject: Sub Discipline-specific Training Guideline for Candidate Medical Equipment Maintainers			
Compiler: MB Mtshali	Approving Officer: EL Nxumalo	Next Review Date: 09/02/2026	Page 34 of 34

Outcome 10: Be responsible for making decisions on part or all of all of one or more <i>specifically-defined</i> engineering activities	Responsibility level E Responsible means “legally or morally liable for carrying out a duty; for the care of something or somebody in a position where one may be blamed for loss, failure, etc.”
Competency Indicators: Responsibility is displayed by the following performance: 10.1 Show how <u>you</u> used HCert level theoretical calculations to justify decisions taken in doing engineering work. Attach actual calculations; 10.2 State how <u>you</u> took responsible advice on any matter falling outside your own education and experience; 10.3 Describe how <u>you</u> took responsibility for your own work and evaluated any shortcoming in your output	10.1 The calculations, for example fault levels, load calculations, losses, return on investment, etc. are done to ensure that the correct material and components are utilized. 10.2 The Specified Category Practitioner does not operate on tasks at a higher level than <i>specifically-defined</i> and consult professionals if elements of the tasks to be done are beyond his/her education and experience, e.g. power system stability, legal actions, etc. 10.3 This is in the first instance continuous self-evaluation to ascertain that the task given is done correctly, on time and within budget. Continuous feedback to the originator of the task instruction, and corrective action if necessary, forms an important element.
Range Statement: Responsibility must be discharged for significant parts of a one or more <i>specifically-defined</i> engineering activity.	The responsibility is mostly allocated within a team environment with an increasing designation as experience is gathered.
Note 1: Responsibility for the evaluation of work in a supervisory capacity.	

Group E: Initial Professional Development (IPD)	Explanation and Responsibility Level
Outcome 11: Undertake independent learning activities sufficient to maintain and extend his or her competence	Responsibility level D
Competency Indicators: Self-development managed by typically: 11.1 Provide <u>your</u> strategy adopted independently to enhance professional development. (IPD report); 11.2 Be aware of the philosophy of employer in regard to professional development.	11.1 If possible, a specific field of the sub-discipline is chosen, available developmental alternatives established, a program drawn up (in consultation with employer if costs are involved), and options open to expand knowledge into additional fields investigated. 11.2 Record keeping must not be left to the employer or anybody else. The trainee must manage his/her own training independently, taking initiative and be in charge of experiential development towards Specified Category Practitioner registration level. Knowledge of the employer’s policy and procedures on training is essential.
Range Statement: Professional development involves: (a) Taking ownership of own professional development; (b) Planning own professional development strategy; (c) Selecting appropriate professional development activities; and (d) Recording professional development strategy and activities; while displaying independent learning ability.	(a) This is <u>your</u> professional development, not the organisation you are working for. (b) In most places of work training is seldom organised by some training department. It is up to the Specified Category Practitioner to manage his/her own experiential development. Specified Category Practitioners frequently end up in a ‘dead-end street’ being left behind doing repetitive work. If self-development is not driven by him/herself, success is unlikely. (c) Preference must be given to engineering development rather than developing soft skills. (d) Developing a learning culture in the workplace environment of the Specified Category Practitioner is vital to his / her success. Information is readily available, and most senior personnel in the workplace are willing to mentor, if approached.

CONTROLLED DISCLOSURE

When downloaded for the ECSA Document Management System, this document is uncontrolled and the responsibility rests with the user to ensure that it is in line with the authorised version on the database. If the 'original' stamp in red does not appear on each page, this document is uncontrolled.